


ENV - 302 RL / ENV - 302HD
INSTALLATION INSTRUCTIONS

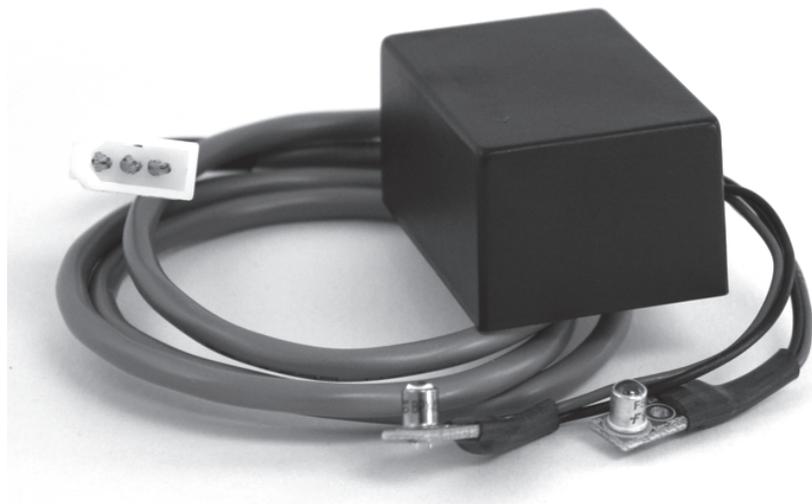

DOC-229
Rev. 1.1


Copyright ©2013
All Rights Reserved

Med Associates Inc.
P.O. Box 319
St. Albans, Vermont 05478


Phone: 802.527.2343
Fax: 802.527.5095
www.med-associates.com

ENV-302RL / ENV-302HD INSTALLATION INSTRUCTIONS


STEP 1: REMOVE THE BLOCK

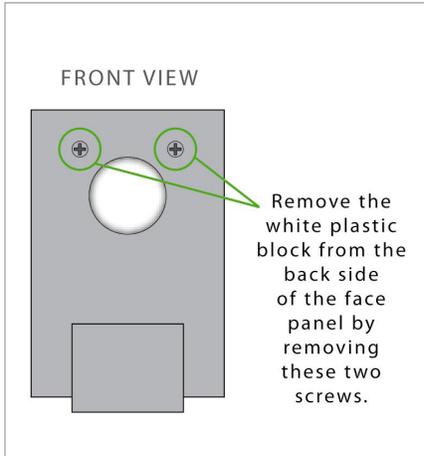

STEP 2: INSTALL THE RECEPTACLE LIGHT

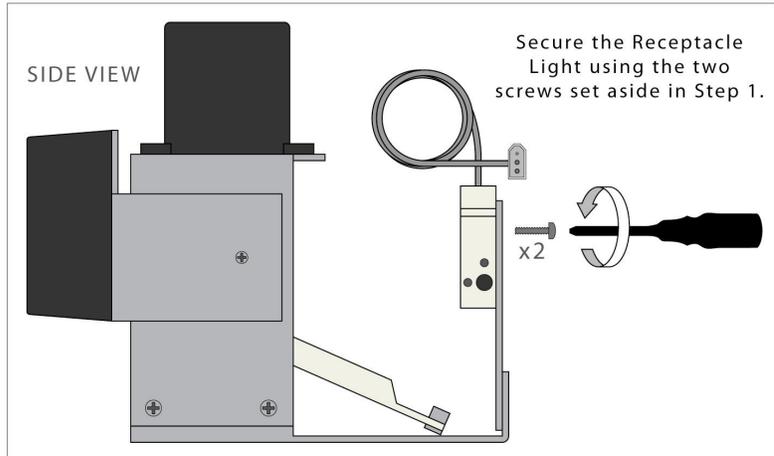

STEP 3: INSTALL THE HEAD ENTRY DETECTOR

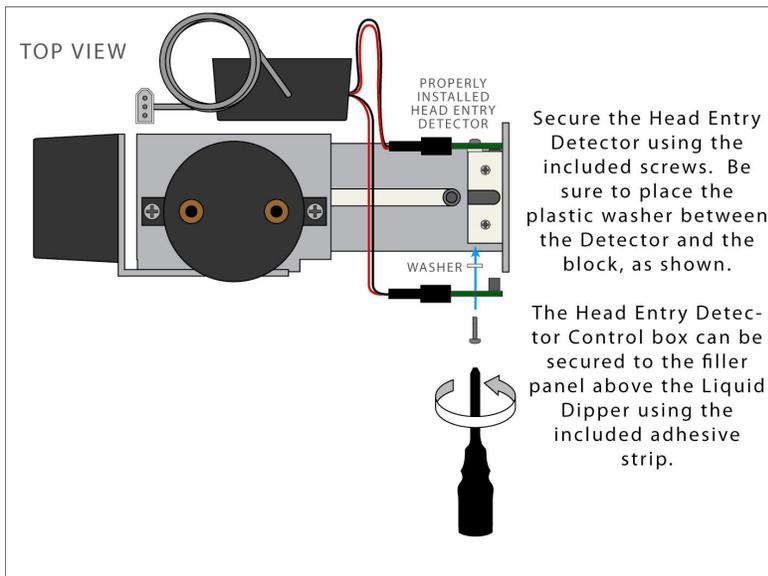

STEP 4: CONNECT TO MED INTERFACE

